

DOCKET NO. 14XZ133155
APPLICATION NO.
INVENTOR: JUENEHOMME ET AL.
TITLE: METHOD AND APPARATUS FOR CALIBRATION AND
CORRECTION OF GRAY LEVELS IN IMAGES
ATTORNEY: JAY L. CHASKIN, REG. NO. 24030; CUSTOMER NO. 23413

1 / 6

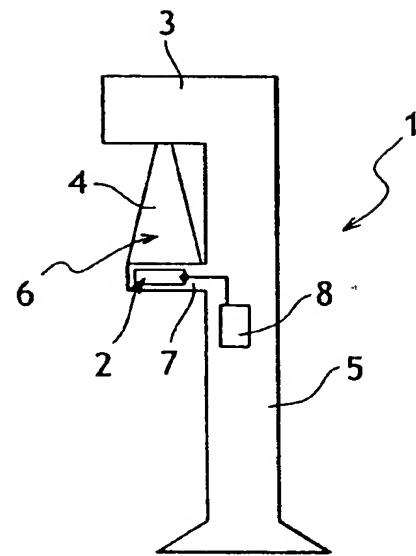


FIG.1

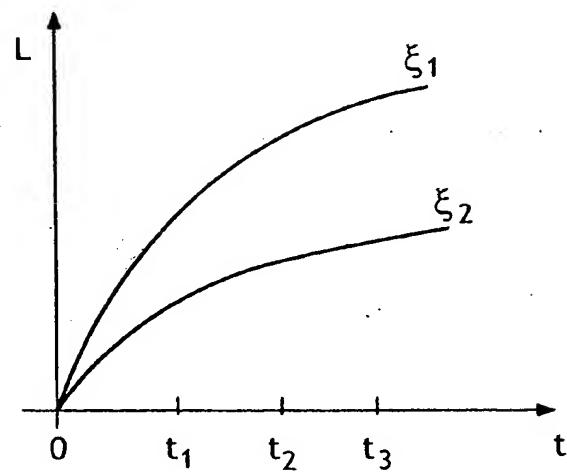


FIG.2

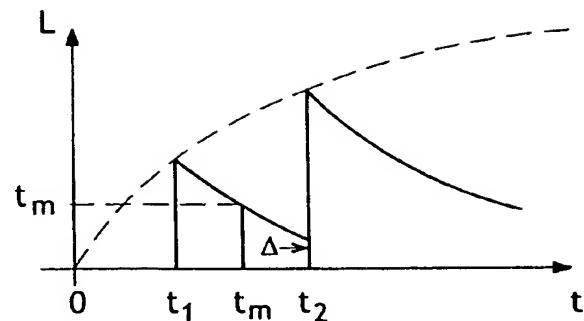


FIG.3

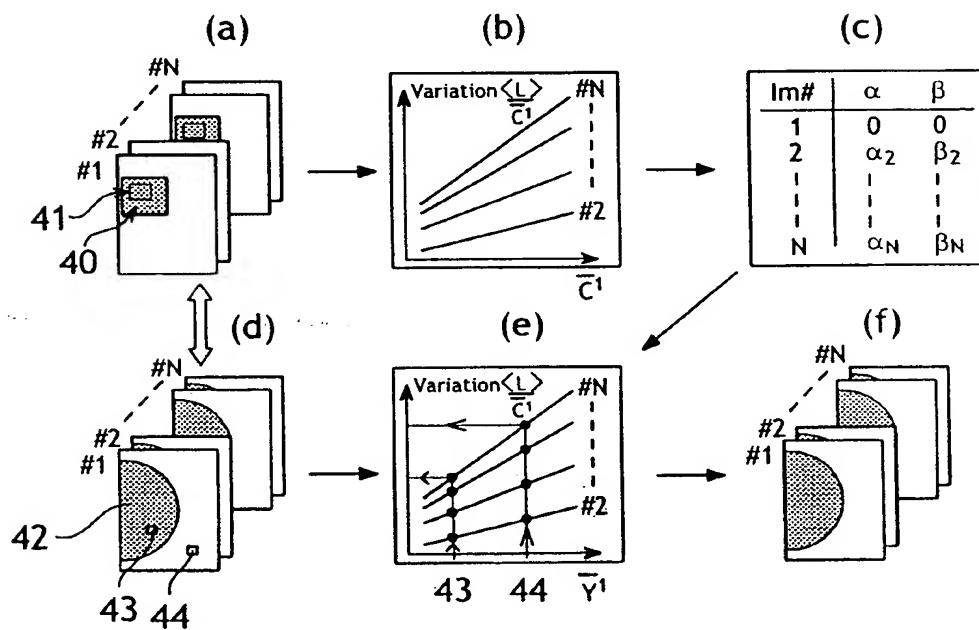


FIG.4

3 / 6

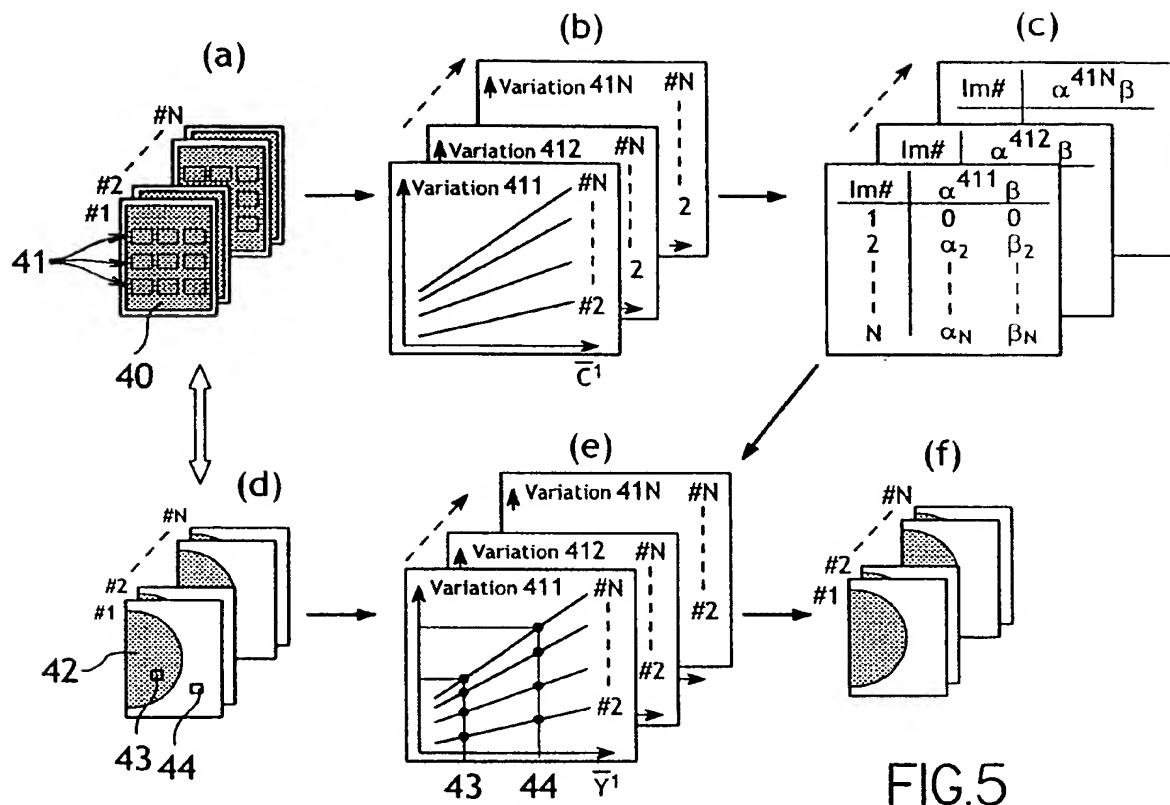


FIG. 5

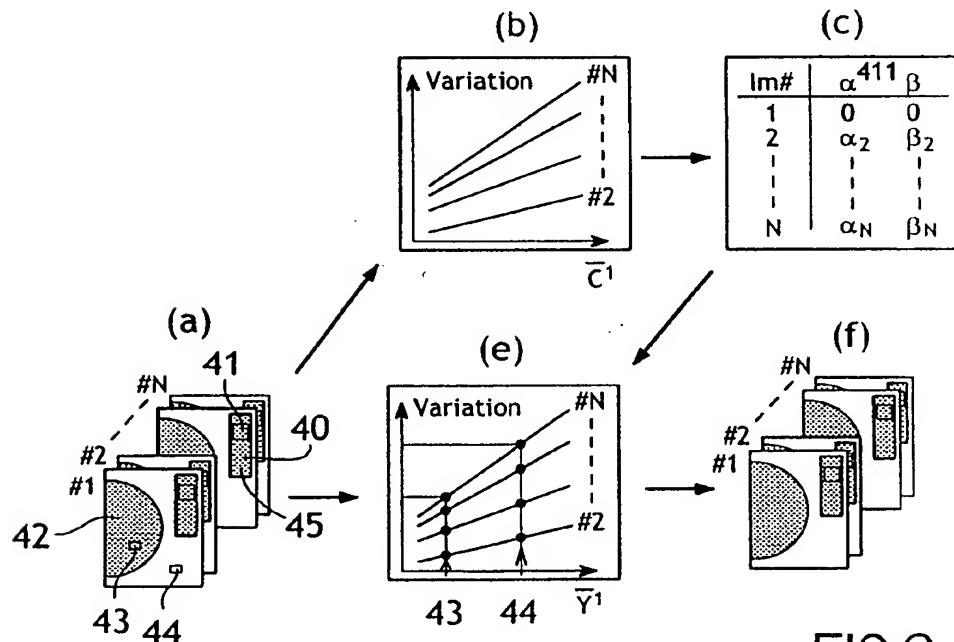


FIG. 6

4 / 6

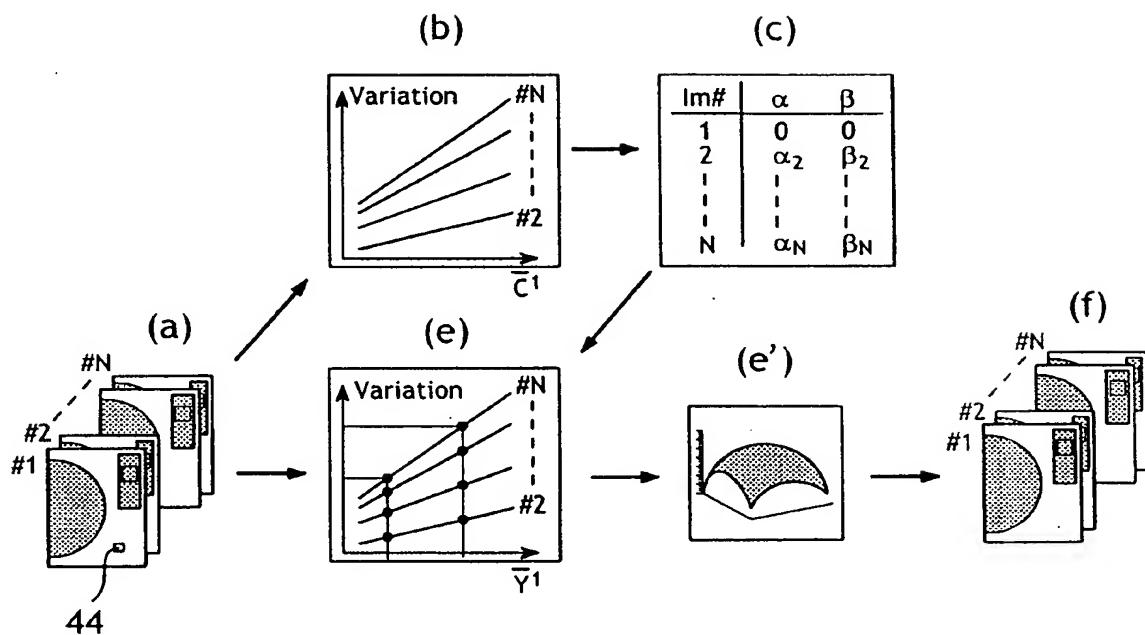


FIG.7

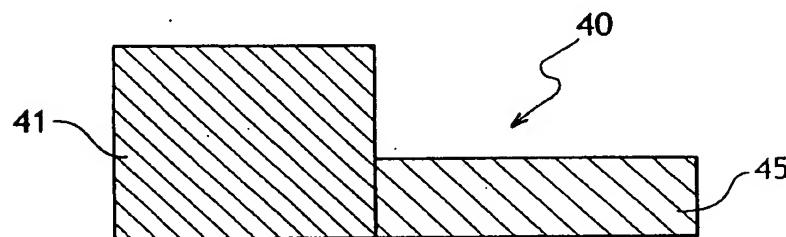


FIG.8

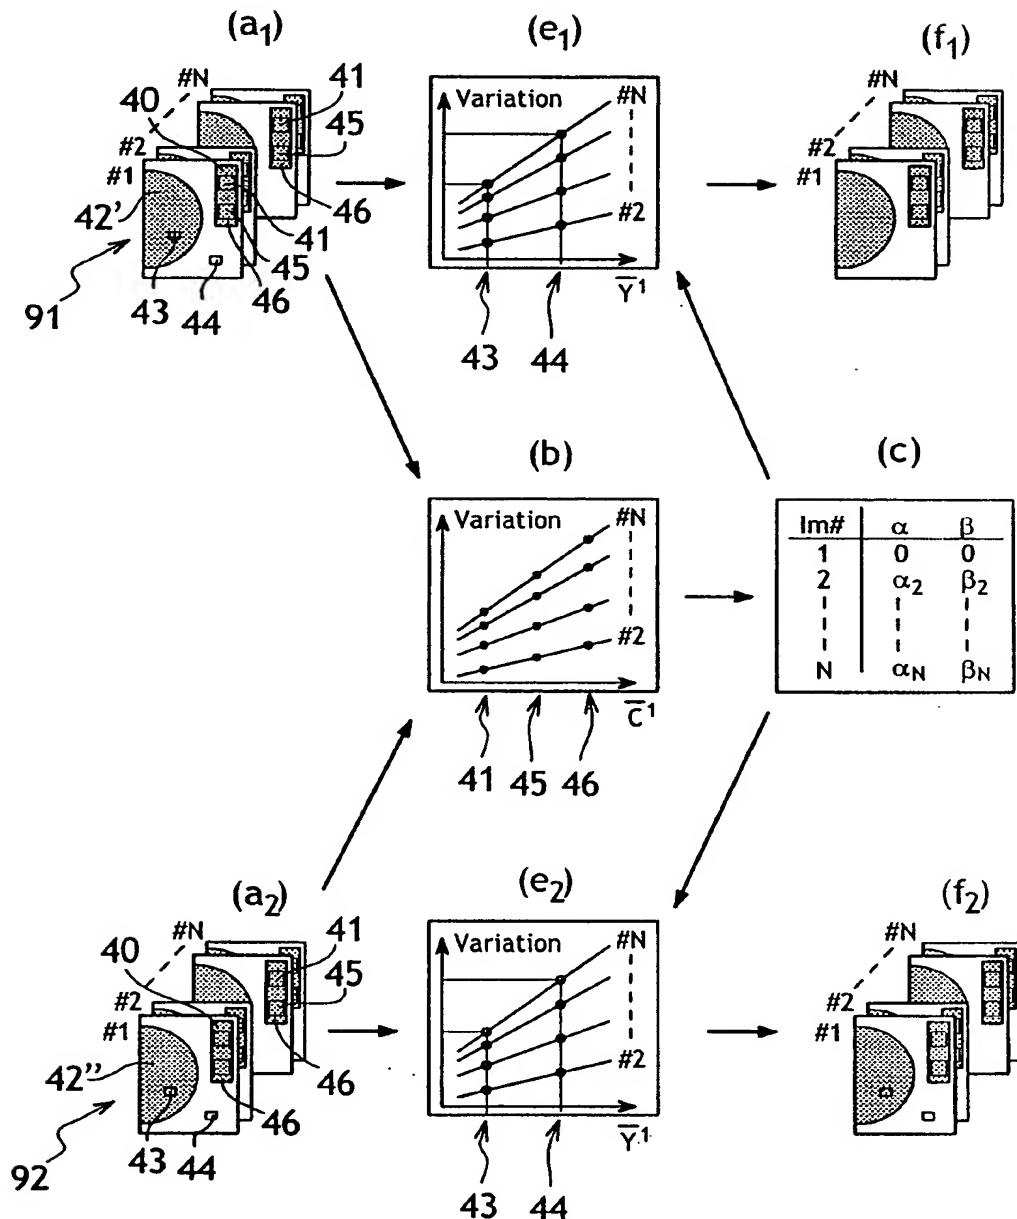


FIG.9

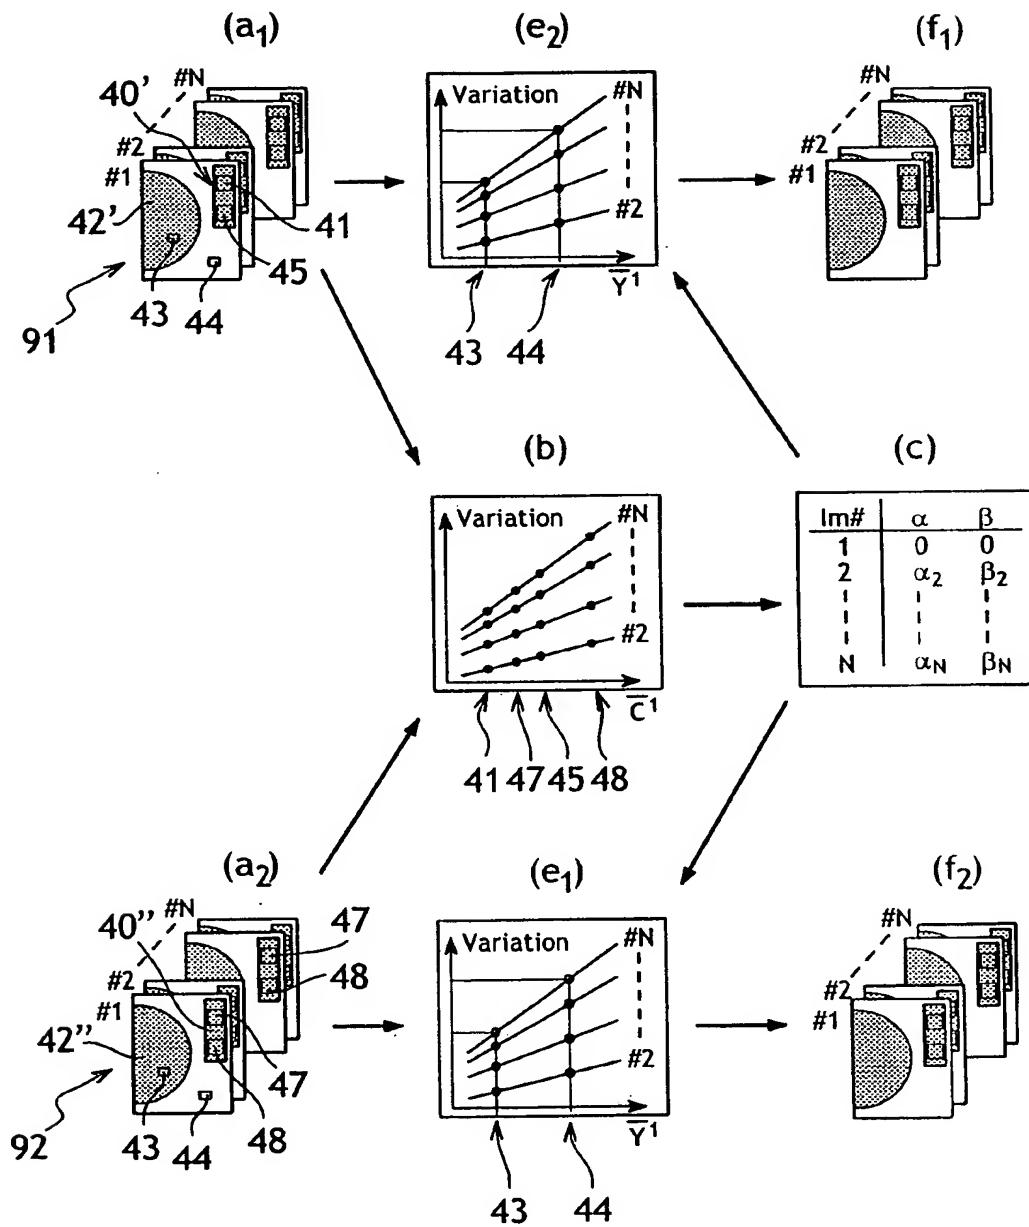


FIG.10